

ARTISS FIBRIN SEALANT- fibrinogen human, human thrombin solution

Baxter Healthcare Corporation

HIGHLIGHTS OF PRESCRIBING INFORMATION

These highlights do not include all the information needed to use ARTISS safely and effectively. See full prescribing information for ARTISS.

ARTISS [Fibrin Sealant (Human)]

Solution for topical application

Initial U.S. Approval: 2008

----- INDICATIONS AND USAGE -----

ARTISS is a fibrin sealant indicated to:

- Adhere autologous skin grafts to surgically prepared wound beds resulting from burns in adult and pediatric populations greater than or equal to 1 year of age (1)
- Adhere tissue flaps during facial rhytidectomy surgery (face-lift) (1)

ARTISS is not indicated as an adjunct to hemostasis (1)

----- DOSAGE AND ADMINISTRATION -----

For topical use only. (2)

Individualize the amount based on the size of the surface to be covered. (2)

- 2 mL will cover approximately 100 cm² surface area
- 4 mL will cover approximately 200 cm² surface area
- 10 mL will cover approximately 500 cm² surface area

Apply a thin layer using the Easyspray and Spray Set or an equivalent device cleared by FDA for application of ARTISS. (2.2)

----- DOSAGE FORMS AND STRENGTHS -----

ARTISS solution is available as a 2 mL, 4 mL, and 10 mL (total volume) pre-filled syringe. (3)

----- CONTRAINDICATIONS -----

- Do not inject directly into the circulatory system (4)
- Do not use in individuals with a known hypersensitivity to aprotinin (4)
- Do not spray where the minimum recommended distance from the applicator tip to the target site cannot be assured (4).

----- WARNINGS AND PRECAUTIONS -----

- Hypersensitivity reactions, including anaphylaxis, can occur. Should symptoms occur, discontinue and administer appropriate treatment. (5.1)
- To reduce the risk of potential life-threatening gas embolism, spray using only the appropriate pressurized gas at the recommended pressure (21.8-29.0 psi) and distance (10-15 cm). Use the **EASYSpray** device connected to a CO₂, Medical Air or Nitrogen CO₂. (5.2)
- ARTISS may denature when exposed to solutions containing alcohol, iodine or heavy metals. (5.3)
- As ARTISS is made from human plasma, it may carry the risk of transmitting infectious agents, e.g., viruses, the variant Creutzfeldt-Jakob disease (vCJD) and theoretically, the classic Creutzfeldt-Jakob disease agent (5.4)

----- ADVERSE REACTIONS -----

Adverse reactions reported during clinical trials in greater than 1% of subjects were:

Burns: Skin graft failure, hematoma and pruritus (6.1)

Facial Rhytidectomy: Hematoma/seroma (6.1)

To report SUSPECTED ADVERSE REACTIONS, contact Baxter Healthcare Corporation at 1-888-229-0001 or FDA at 1-800-FDA-1088 or www.fda.gov/medwatch.

----- USE IN SPECIFIC POPULATIONS -----

Pregnancy: No human or animal data. Use only if deemed clinically necessary. (8.1)

See 17 for PATIENT COUNSELING INFORMATION.

Revised: 12/2019

FULL PRESCRIBING INFORMATION: CONTENTS*

1 INDICATIONS AND USAGE

2 DOSAGE AND ADMINISTRATION

2.1 Preparation

2.2 Method of Application

3 DOSAGE FORMS AND STRENGTHS

4 CONTRAINDICATIONS

5 WARNINGS AND PRECAUTIONS

5.1 Hypersensitivity Reactions

5.2 Application Precautions

5.3 Protein Denaturation

5.4 Transmission of Infectious Agents

6 ADVERSE REACTIONS

6.1 Clinical Trials Experience

6.2 Post-Marketing Experience

7 DRUG INTERACTIONS

8 USE IN SPECIFIC POPULATIONS

8.1 Pregnancy

8.2 Lactation

8.3 Females and Males of Reproductive Potential

8.4 Pediatric Use

8.5 Geriatric Use

10 OVERDOSAGE

11 DESCRIPTION

12 CLINICAL PHARMACOLOGY

12.1 Mechanism of Action

12.2 Pharmacodynamics

14 CLINICAL STUDIES

16 HOW SUPPLIED/STORAGE AND HANDLING

17 PATIENT COUNSELING INFORMATION

* Sections or subsections omitted from the full prescribing information are not listed.

FULL PRESCRIBING INFORMATION

1 INDICATIONS AND USAGE

ARTISS is a fibrin sealant indicated to:

- Adhere autologous skin grafts to surgically prepared wound beds resulting from burns in adult and pediatric populations greater than or equal to 1 year of age.
- Adhere tissue flaps during facial rhytidectomy surgery (face-lift).

ARTISS is not indicated as an adjunct to hemostasis.

2 DOSAGE AND ADMINISTRATION

For topical use only.

2.1 Preparation

Do not expose to temperatures above 37°C.

Do not microwave.

Do not refrigerate or re-freeze after thawing.

Do not use ARTISS unless it is completely thawed and warmed to 33°C-37°C.

Do not remove the protective syringe cap until thawing is complete and the application tip is ready to be attached.

Room Temperature Thawing

Unopened pouches can be stored for up to 14 days at 15°C to 25°C. Before use, warm the product to 33°C- 37°C.

Table 1 Approximate Room Temperature Thawing and Incubator Warming Times

Pack Size in Pouch	Room Temperature (In Pouches) 15 °C to 25°C	Warming thawed pouches prior to use 33°C to 37°C Incubator
2 mL	60 minutes	15 minutes
4 mL	110 minutes	25 minutes
10 mL	160 minutes	35 minutes

Quick Thawing

Sterile Water Bath (Quick Thawing): Transfer inner pouch to the sterile field, remove pre-filled syringe from inner pouch and place directly into sterile water bath ensuring the syringe is completely immersed in the water. Maintain the product at 33°C to 37°C until use. If the package is opened or warmed to 33°C to 37°C, it must be used within 12 hours.

Non-Sterile Water Bath: Maintain the pre-filled syringe in pouches and place into a water bath outside the sterile field ensuring the pouches remain submerged. Remove from the water bath after thawing and warming, dry the external pouch and transfer inner pouch with pre-filled syringe onto the sterile field. Maintain the product at 33°C to 37°C until use. If the package is opened or warmed to 33°C to 37°C, it must be used within 12 hours.

Incubator: Maintain the pre-filled syringe in pouches and place into an incubator. Remove from the incubator after thawing and warming. Transfer inner pouch with pre-filled syringe onto the sterile field. Maintain the product at 33°C to 37°C until use. If the package is opened or warmed to 33°C to 37°C, it must be used within 12 hours.

Table 2 Approximate Water Bath or Incubator Thawing and Warming Times

Pack Size in Pouch	Sterile Water Bath (Pouches Removed) 33 °C to 37°C	Non-Sterile Water Bath (In Pouches) 33 °C to 37°C	Incubator (In Pouches) 33 °C to 37°C
2 mL	5 minutes	30 minutes	40 minutes
4 mL	5 minutes	40 minutes	85 minutes
10 mL	12 minutes	80 minutes	105 minutes

2.2 Method of Application

ARTISS must be applied only to application sites that are visible. Individualize the amount to be applied based on the size of the surface to be covered. Prior to applying ARTISS, dry the site of application using standard techniques (e.g., intermittent application of compresses, swabs, use of suction devices).

Do not use pressurized air or gas for drying the site. Apply ARTISS as a thin layer.

The approximate surface areas covered by each package size are:

Table 3

Approximate area requiring skin graft fixation	Required package size of ARTISS
100 cm ²	2 mL
200 cm ²	4 mL
500 cm ²	10 mL

When applying ARTISS using a spray device, utilize the recommended gas, pressure and distance from tissue within the ranges recommended by the manufacturer as follows:

Table 4: Recommended Application Equipment, Gas and Parameters.

Surgery	Spray set / Applicator tips to use	Pressure regulator to use	Gas	Distance	Spray Pressure
Open surgery	Tisseel / Artiss Spray Set	EasySpray Regulator	CO ₂ *, Medical Air or Nitrogen	10-15 cm	1.5-2.0 bar (21.8-29.0 psi)

* CO₂ is the preferred gas for application, however Medical Air or Nitrogen are acceptable gasses for administration of ARTISS in open surgery.

Application with Spray Device

Apply using the EasySpray and Spray Set, or an equivalent device cleared by FDA for application of ARTISS. See additional instructions for use provided with the spray set. Artiss must not be used with the EasySpray / Spray set system in enclosed body cavities.

Ensure that parts of the body outside the desired application area are sufficiently covered to prevent tissue adherence at undesired site.

Apply as a thin layer to avoid the formation of excess granulation tissue and to ensure gradual absorption of the polymerized fibrin sealant. Excessive clot thickness may delay the natural wound healing process. Ensure that the amount applied is sufficient to entirely cover the intended application area.

The aerosolized sealant should be applied to the wound in a painting motion from side to side to achieve an even thin layer. The wound bed will glisten in the area to which fibrin sealant has been applied. Any areas not covered by fibrin sealant will be clearly visible.

Attach the skin flap or graft to the wound bed immediately after ARTISS has been sprayed. Wet gloves with normal saline before product contact to prevent adherence. The surgeon has up to 60 seconds to manipulate and position the flap or graft prior to polymerization.

Repeat application, if necessary, to any small areas that may not have been previously treated.

Hold the flap or graft in the desired position by gentle compression for at least 3 minutes to ensure ARTISS sets properly and firmly adheres the skin graft or flap to the underlying tissue. The solidified fibrin sealant reaches its final strength in approximately 2 hours after application.

Application with DUO Set A

The cannulas included with the DUO Set A may be used for small wounds or for edges of a skin graft that did not adhere to the wound bed [see *Warnings and Precautions (5.3)*]. Immediately before application, expel and discard the first several drops from the application cannula to ensure adequate

mixing of the Sealer Protein and Thrombin solutions in cases where very small volumes (1-2 drops) are administered.

DUO Set A Instructions (see Figure 1 below):

1. Insert plunger into syringe barrel.
2. Firmly connect the two syringe nozzles to the joining piece and secure it by fastening the tether strap to the syringe.
3. Fit an application cannula to the joining piece.

Note: Interruption of application causes clogging in the cannula. Replace the cannula immediately prior to resuming application. If the opening of the joining piece (Y connector) facing the cannula is clogged, use the spare joining piece provided in the package.

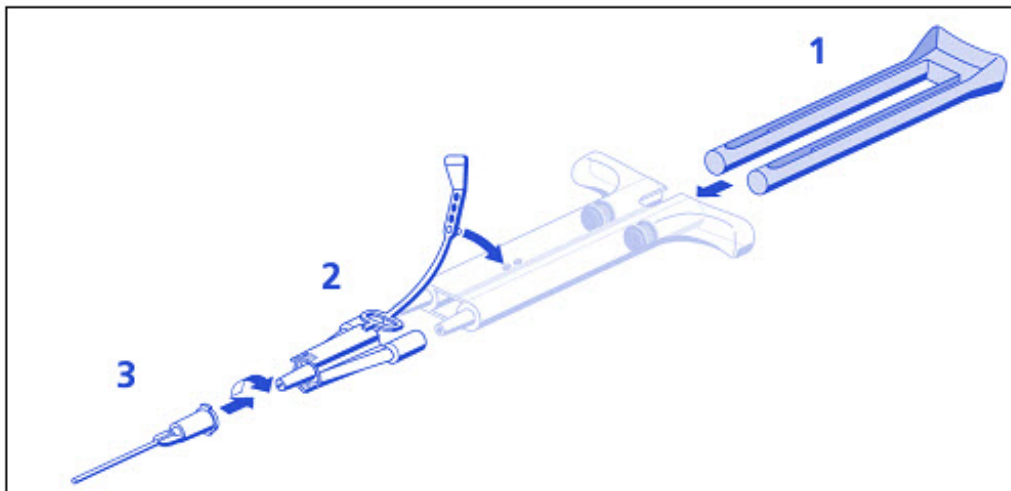


Figure 1 DUO Set A

Pre-filled syringes are for single use only. Discard unused contents.

3 DOSAGE FORMS AND STRENGTHS

ARTISS is a two component fibrin sealant solution, comprised of sealer protein (human) and thrombin (human) available in a 2 mL, 4 mL, or 10 mL (total volume) pre-filled syringe with the DUO Set A.

4 CONTRAINDICATIONS

Do not inject directly into the circulatory system or into highly vascularized tissue. Intravascular application can result in life-threatening thromboembolic events and can increase the likelihood and severity of acute hypersensitivity reaction in susceptible patients.

Do not use in individuals with a known hypersensitivity to aprotinin and/or hypersensitivity to any of the active substances or excipients of ARTISS including proteins such as fibrinogen, thrombin, and human albumin [see *Warnings and Precautions (5.1)* and *Adverse Reactions (6)*].

Do not spray where the minimum recommended distance from the applicator tip to the target site cannot be assured.

5 WARNINGS AND PRECAUTIONS

5.1 Hypersensitivity Reactions

Hypersensitivity reactions, including anaphylaxis, can occur. Cases have been reported in post-marketing experience with fibrin sealant. In specific cases, these reactions have progressed to anaphylaxis. Such reactions may especially be seen if product is applied repeatedly over time or in the same setting, or if systemic aprotinin has been administered previously; however, these reactions may also occur in patients receiving ARTISS for the first time. A first successful treatment does not exclude a later allergic reaction. Symptoms associated with allergic anaphylactic reactions include: Flushing, urticaria, pruritus, nausea, drop in blood pressure, tachycardia or bradycardia, dyspnea, severe hypotension and anaphylactic shock.

Aprotinin, a monomeric polypeptide, is known to be associated with anaphylactic reactions. Even in the case of strict local application of aprotinin, there is a risk of anaphylactic reactions to aprotinin, particularly in the case of previous exposure [see *Contraindications (4)*].

Discontinue administration in the event of hypersensitivity reactions. Remove the already applied, polymerized product from the surgical field. Mild reactions can be managed with antihistamines. Severe reactions and reactions involving hypotension require immediate resuscitative intervention.

5.2 Application Precautions

Any application of pressurized air or gas is associated with a potential risk of air or gas embolism, tissue rupture, or gas entrapment with compression, which may be life threatening or fatal.

Life threatening/fatal air or gas embolism has occurred with the use of spray devices employing pressure regulator to administer fibrin sealants. This can occur if a spray device is used at higher than recommended pressures and in closer than recommended proximity to the tissue surface. The risk appears to be higher when fibrin sealants are sprayed with air, as compared to CO₂ and therefore cannot be excluded with ARTISS when sprayed in open surgical procedures.

To reduce the risk of a potentially life-threatening gas embolism when using a spray device, be sure to use the pressure within the pressure range recommended by the spray device manufacturer. In the absence of a specific recommendation avoid using pressure above 20-25 psi. Do not spray closer than the distance recommended by the spray device manufacturer. In the absence of a specific recommendation avoid spraying closer than 10-15 cm from the surface of the tissue. When spraying, changes in blood pressure, pulse, oxygen saturation and end tidal CO₂ should be monitored because of the possibility of occurrence of air or gas embolism. When using the EasySpray device, or an equivalent spray device cleared by FDA, use the pressure within the pressure range recommended by the spray device manufacturer. Spray only on to visible application sites, not in enclosed body cavities.

5.3 Protein Denaturation

The sealer protein and thrombin solutions can be denatured by alcohol, iodine or heavy metal ions (e.g., antiseptic solutions). If any of these substances have been used to clean the wound area, the area must be thoroughly rinsed before application of ARTISS and made as dry as possible.

5.4 Transmission of Infectious Agents

ARTISS is made from human plasma. Because this product is made from human blood, it may carry a risk of transmitting infectious agents, e.g., viruses, the variant Creutzfeldt-Jakob disease (vCJD) agent, and theoretically, the Creutzfeldt-Jakob disease (CJD) agent. All infections thought by a physician possibly to have been transmitted by this product should be reported by the physician or other healthcare provider to Baxter Healthcare Corporation, telephone no. 1-888-229-0001.

Some viruses, such as parvovirus B19, are particularly difficult to remove or inactivate at this time. Parvovirus B19 most seriously affects pregnant women (fetal infection), immune-compromised individuals or individuals with an increased erythropoiesis (e.g., hemolytic anemia) [see *Pregnancy (8.1)* and *Patient Counseling Information (17)*].

6 ADVERSE REACTIONS

The most frequent ($\geq 1\%$ of clinical trial subjects) adverse reactions with the use of ARTISS were: Skin graft failure, hematoma and pruritus in burn studies, and hematoma/seroma in rhytidectomy studies.

6.1 Clinical Trials Experience

Because clinical trials are conducted under widely varying conditions, adverse reaction rates observed in the clinical trials of a drug cannot be directly compared to rates in the clinical trials of another drug and may not reflect the rates observed in practice.

The burn and rhytidectomy surgery trials were prospective, randomized, controlled, multicenter clinical trials with a total of 298 subjects. In each trial, the subject served as its own control. All subjects treated have been included into the safety analysis. [see *Clinical Studies (14)*]

The data described in Table 5 reflects the exposure to ARTISS in the 4 burn and rhytidectomy surgery trials:

Table 5

Trial Population Demographics				
	Burn		Rhytidectomy	
Parameter	Preliminary Trial	Confirmatory Trial	Preliminary Trial	Confirmatory Trial
Sample size (N)	40	138	45	75
Gender	11 (27.5%)	44 (31.9%)	42 (93.3%)	71 (94.7%)
F (%) /	29 (72.5%)	94 (68.1%)	3 (6.7%)	4 (5.3%)
M (%)				
Age Range (years)	6-55	1-63	43-70	40-71
Volume applied (Mean \pm SD) (Range in mL)	2.9 \pm 1.64 (Range: 1.0-10.8)	2.7 \pm 1.9 (Range: 0.2-12.0)	2.32 \pm 0.95 (Range: 0.80-4.0)	2.58 \pm 1.17 (Range: 0.60-4.0)

Adverse reactions in the burn trials occurring in greater than 1% of subjects were skin graft failure (3%), hematoma (1%) and pruritus (1%) [n=178].

Adverse reactions in the facial rhytidectomy trials occurring in greater than 1% of subjects were hematoma/seroma (4%) [n=120].

6.2 Post-Marketing Experience

Air embolism

As with other fibrin sealants, life threatening/fatal air or gas embolism may occur when using devices with pressurized air or gas occurred; this event appears to be related to an inappropriate use of the spray device (e.g. at higher than recommended pressures (21.8-29.0 psi) and/or in close proximity to the tissue surface (10-15 cm)).

7 DRUG INTERACTIONS

Oxycellulose containing preparations may reduce the efficacy of ARTISS and should not be used as carrier materials. No interaction studies have been performed.

8 USE IN SPECIFIC POPULATIONS

8.1 Pregnancy

Risk Summary

There are no available data on ARTISS use in pregnant women to inform a drug-associated risk of adverse developmental outcomes. Animal reproduction studies have not been conducted. It is also not known whether ARTISS can cause fetal harm when administered to a pregnant woman or can affect reproduction capacity. Some viruses, such as parvovirus B19, are particularly difficult to remove or inactivate at this time. Parvovirus B19 most seriously affects pregnant women (fetal infection). ARTISS should be given to a pregnant woman only if deemed medically necessary.

The estimated background risk of major birth defects and miscarriage for the indicated populations are unknown. All pregnancies have a background risk of birth defect, loss, or other adverse outcomes. In the U.S. general population, the estimated background risk of major birth defects and miscarriage in clinically recognized pregnancies is 2-4% and 15-20%, respectively.

Clinical Considerations

ARTISS use in pregnant woman should be assessed for benefit and risk probability and used when deemed clinically necessary.

8.2 Lactation

Risk Summary

There are no direct or controlled studies of ARTISS in lactating women. It is not known whether this drug is excreted in human milk, there is no information regarding the effects on the breastfed infant, and the effects on milk production. Because many drugs are excreted in human milk, caution should be exercised when administered to lactating mothers.

The developmental and health benefits of breastfeeding should be considered along with the mother's clinical need for ARTISS and any potential adverse effects on the breastfed child from ARTISS or from underlying maternal condition.

8.3 Females and Males of Reproductive Potential

Infertility

No direct clinical studies have been conducted to evaluate safety and efficacy of ARTISS in infertility. There is limited data from case reports with fibrin sealant use in both male and female infertility. The general outcome from ARTISS use has not indicated the product as a source of safety concern or lack of effectiveness for its labeled indication in these population groups.

8.4 Pediatric Use

In two clinical trials utilizing ARTISS to adhere autologous skin grafts to surgically prepared wound beds resulting from burns, the efficacy and safety in 38 pediatric subjects (27 subjects ages 1-10 years and 11 subjects ages 11-16 years) were not different from an adult population.

8.5 Geriatric Use

Thirteen subjects aged 65 and older (65-71 years of age) have been treated with ARTISS in facial rhytidectomy clinical trials. Separate evaluations of these subjects were not performed.

10 OVERDOSAGE

To avoid the formation of excess granulation tissue and to ensure gradual absorption of the polymerized fibrin sealant, apply only a thin layer [*Dosage and Administration (2.2)*].

11 DESCRIPTION

ARTISS [Fibrin Sealant (Human)] is a two-component fibrin sealant made from pooled human plasma.
 Sealer Protein Solution

Total protein: 96 -125 mg/mL
 Fibrinogen: 67 - 106 mg/mL
 Fibrinolysis Inhibitor (Synthetic): 2250 - 3750 Kallidinogenase Inhibiting Unit/mL

Other ingredients include: Human albumin, tri-sodium citrate, histidine, niacinamide, polysorbate 80 and water for injection (WFI).

Thrombin Solution

Thrombin (Human): 2.5 - 6.5 units/mL¹
 Calcium Chloride: 36 - 44 µmol/mL

Other ingredients include: Human albumin, sodium chloride and water for injection (WFI).

Sealer Protein (Human)

Sealer Protein (Human) is a sterile, non-pyrogenic, vapor-heated and solvent/detergent treated preparation made from pooled human plasma. Sealer Protein (Human) is provided as a frozen liquid solution pre-filled into one side of a dual-chambered syringe (1). The active ingredient in Sealer Protein (Human) is fibrinogen. A Fibrinolysis Inhibitor, Aprotinin (Synthetic) is included in the Sealer Protein (Human) component to delay fibrinolysis. Aprotinin (Synthetic) is manufactured by solid phase synthesis from materials completely of non-human/non-animal origin.

Thrombin (Human)

Thrombin (Human) is a sterile, non-pyrogenic, vapor-heated and solvent/detergent treated preparation made from pooled human plasma. Thrombin (Human) is provided as a frozen liquid solution pre-filled into one side of a dual-chambered syringe (2).

Sealer Protein (Human) and Thrombin (Human) are made from pooled human plasma collected at US licensed collection centers. The vapor heat and solvent/detergent treatment steps used in the manufacturing process have been shown to be capable of significant viral reduction. No procedure, however, has been shown to be completely effective in removing viral infectivity from derivatives of human plasma [see *Viral Clearance* below and *Warnings and Precautions (5.4)*].

Viral Clearance

The manufacturing procedure includes processing steps designed to further reduce the risk of viral transmission. In particular, vapor heating and solvent/detergent treatment processes are included in the manufacturing of Sealer Protein Concentrate and Thrombin. Validation studies were conducted using samples drawn from manufacturing intermediates for each of the two human plasma derived components. These samples were spiked with stock virus suspensions of known titers followed by further processing under conditions equivalent to those in the respective manufacturing steps. The stock virus suspensions represent HIV, HBV, HCV, HAV and Human Parvovirus B19.

The virus reduction factors (expressed as log₁₀) of independent manufacturing steps are shown in Table 6 for each of the viruses tested:

Table 6

Reduction Factors for Virus Removal and/or Inactivation Sealer Protein Component					
Manufacturing Step	Mean Reduction Factors [log ₁₀] of Virus Tested				
	HIV-1	HAV	BVDV	PRV	MMV

Early Manufacturing Steps	n.d.	n.d.	n.d.	n.d.	2.7
Solvent/Detergent Treatment	>5.3	n.d.	>5.7	>5.9	n.d.
Vapor Heat Treatment	>5.5	>5.6	>5.7	>6.7	1.2
Overall Reduction Factor (ORF)	>10.8	>5.6	>11.4	>12.6	3.9
Reduction Factors for Virus Removal and/or Inactivation Thrombin Component					
	Mean Reduction Factors [\log_{10}] of Virus Tested				
Manufacturing Step	HIV-1	HAV	BVDV	PRV	MMV
Thrombin precursor mass capture	3.2	1.5	1.8	2.5	1.2
Vapor Heat Treatment	>5.5	>4.9	>5.3	>6.7	1.0
Solvent/Detergent Treatment	>5.3	n.d.	>5.5	>6.4	n.d.
Ion Exchange Chromatography	n.d.	n.d.	n.d.	n.d.	3.6
Overall Reduction Factor (ORF)	>14.0	>6.4	>12.6	>15.6	5.8

n.d. = not determined

HIV-1: Human immunodeficiency virus 1; **HAV:** Hepatitis A virus; **BVDV:** Bovine viral diarrhea virus, a model for Hepatitis C virus; **PRV:** Pseudorabies virus, a model for enveloped DNA viruses, among those Hepatitis B virus; **MMV:** Mice minute virus, a model for B19V.

In addition, Human Parvovirus B19 was used to investigate the upstream Thrombin precursor mass capture step, the Sealer Protein early manufacturing steps and the Thrombin and Sealer Protein vapor heating steps. Using quantitative PCR assays, the estimated log reduction factors obtained were 1.7 and 3.4 for the Thrombin precursor mass capture step and Sealer Protein early manufacturing steps and >4 / 1.0 for the Thrombin / Sealer Protein vapor heating steps, respectively.

¹ The potency expressed in units is determined using a clotting assay against an internal reference standard for potency that has been calibrated against the World Health Organization (WHO) Second International Standard for Thrombin, 01/580. Therefore, a unit is equivalent to an International Unit (IU).

12 CLINICAL PHARMACOLOGY

12.1 Mechanism of Action

Upon mixing Sealer Protein (Human) and Thrombin (Human), the two components mimic the final stage of the blood coagulation cascade. Soluble fibrinogen is transformed into fibrin that adheres to the wound surface and to the skin flap or graft to be affixed. Due to the low thrombin concentration, initial polymerization will take up to 60 seconds. The fibrin clot continues to strengthen for up to 2 hours after application.

Spray application over the wound bed provides full surface adherence of skin flaps and grafts. Full surface adherence minimizes areas of dead space between the wound bed and applied tissues. Elimination of dead space prevents shear irritation upon movement as well as reduces the void space under the skin that can host fluid build-up.

12.2 Pharmacodynamics

Thrombin is a highly specific protease that transforms the fibrinogen contained in Sealer Protein (Human) into fibrin.

Fibrinolysis Inhibitor, Aprotinin (Synthetic), is a polyvalent protease inhibitor that prevents premature

degradation of fibrin. Free Aprotinin and its metabolites have a half-life of 30 to 60 minutes and are eliminated by the kidney. Preclinical studies with different fibrin sealant preparations simulating the fibrinolytic activity generated by extracorporeal circulation in patients during cardiovascular surgery have shown that incorporation of aprotinin in the product formulation increases resistance of the fibrin sealant clot to degradation in a fibrinolytic environment.

14 CLINICAL STUDIES

Burns (grafts)

ARTISS was investigated for adherence of split thickness sheet skin grafts in burn patients in a prospective, randomized, controlled, evaluator-blinded, multicenter clinical trials. In each of the 138 patients, two comparable test sites were identified after burn wound excision. Skin grafts were adhered at one test site using ARTISS, and at the other test site using staples (control). The study product was applied once to the wound bed of the allocated test site during skin grafting surgery.

The mean \pm standard deviation (SD) estimated total body surface area (TBSA) for all burn wounds was $13.6 \pm 9.2\%$. The mean \pm SD estimated TBSA requiring skin grafting was $8.0 \pm 6.9\%$. The mean \pm SD estimated TBSA for ARTISS test sites was $1.7 \pm 0.8\%$ and for the stapled test sites was $1.7 \pm 0.7\%$. Burn wound thickness was classified as full thickness in 106 (76.8%) of the 138 treated subjects, and partial thickness in 32 (23.2%) subjects.

The safety population contained all 138 treated subjects; however, 11 subjects did not have an available primary endpoint assessment, leaving a modified intent-to-treat (ITT) set of 127 patients. Complete wound closure by Day 28 was achieved in 43.3% of the ARTISS test sites and 37.0% of the stapled test sites in the 127 ITT patients. Wound closure at Day 28 was complete at 72% of the ARTISS and staples test sites for the 1-6 years old group (N=18), at 32% of the ARTISS test sites and 26% of the staples test sites for the 7-18 years old group (N=19) and at 40% of the ARTISS test sites and 32% of the staples test sites for the greater than 18 years old group [ITT]. The lower limit of the 97.5% confidence interval of the difference between ARTISS and staples was -0.029. A similar result was obtained in the per protocol (PP) population: complete wound closure by Day 28 was achieved in 45.3% of the ARTISS test sites and 39.6% of the stapled test sites in the 106 PP patients. The lower limit of the 97.5% confidence interval of the difference between ARTISS and staples was -0.041. Therefore, ARTISS was found to be non-inferior to staples in the ITT and PP populations at the 97.5% one-sided level for complete wound closure by Day 28 because the lower limit of the confidence interval of the difference between ARTISS and staples success rates was greater than the predefined limit of -0.1.

Facial Rhytidectomy (flaps)

ARTISS was investigated for adherence of skin flaps in facial rhytidectomy surgeries during two prospective, randomized, controlled, multicenter clinical trials. Both the preliminary trial investigating 45 subjects and the confirmatory trial with 75 subjects had a split-face design in which 1 side of the face was treated with ARTISS as an adjunct to the standard of care (SoC) and the other side received SoC only, which was closure of the flap by means of staples and suturing only; therefore each subject participated in both arms (ARTISS and SoC).

Primary endpoint of the confirmatory trial conducted in 75 subjects was the total drainage volume collected from each side of the face at 24 h (± 4 h) post surgery. Occurrence of hematoma and seroma on each side of the face, comparison of edema between the 2 sides of the face, changes in skin sensitivity from baseline on each side of the face and subject preference were evaluated as secondary endpoints.

In both trials, a standardized drain was placed in each side of the face prior to the flap closure and drainage volume from both sides of the face from all subjects was compared. Pressure dressings were not allowed.

The results for the primary endpoint of the confirmatory trial are presented in Table 7a below.

Table 7a Drainage Volume Comparison at 24 h Post Operative in Confirmatory Trial

Clinical Trial (n=75)	Mean ± SD Drainage (mL) ARTISS Side of the Face	Mean ± SD Drainage (mL) SoC Side of the Face	p-Value
Confirmatory trial	7.7 ± 7.4	20.0 ± 11.3	<0.0001

A statistically significant difference in drainage volumes was observed, favoring the side of the face treated with ARTISS.

Drainage volumes at 24 h post operatively for each side of the face reported as secondary endpoint in the preliminary trial are presented in Table 7b below.

**Table 7b
Drainage Volume Comparison at 24 h Post Operative in Preliminary Trial**

Clinical Trial (n=45)	Mean ± SD Drainage (mL) ARTISS Side of the Face	Mean ± SD Drainage (mL) SoC Side of the Face
Preliminary trial	11.5 ± 13.7	26.8 ± 24.0

An integrated analysis of the occurrence of hematoma/seroma in all 120 subjects across two trials was performed. A comparison of the proportion of subjects experiencing a hematoma/seroma exclusively on the ARTISS-treated side or on the SoC side of the face is presented in Table 8 below.

Table 8 Occurrence of Hematoma/Seroma

Clinical Trial	ARTISS n (%)	SoC n (%)	Both Sides of Face n (%)	Total n (%)
Preliminary trial	0	9 (20%)	0	9 (20%)
Confirmatory trial	2 (2.7%)	5 (6.7%)	3 (4%)	10 (13.3%)

16 HOW SUPPLIED/STORAGE AND HANDLING

Table 9

Pack Size	Packaging Component	NDC
2 mL	Carton	0338-8503-02
	Pouch	0338-8503-01
4 mL	Carton	0338-8503-04
	Pouch	0338-8503-03
10 mL	Carton	0338-8503-10
	Pouch	0338-8503-09

Storage

Store in original carton to protect from light. Do not use after the expiration date. Discard if packaging of any component is damaged.

- Long term: Store at ≤ -20°C.
- Short term: Room Temperature Thawing: Unopened pouches, thawed at room temperature, may be

stored for up to 14 days at room temperature (15°C to 25°C) after removal from the freezer.
Quick Thawing: Maintain the product at 33°C to 37°C until use. If the product is removed from original pouch or warmed to 33°C to 37°C it must be used within 12 hours.

Do not refrigerate or re-freeze after thawing. Do not microwave.

17 PATIENT COUNSELING INFORMATION

Inform patients that ARTISS is made from human plasma and discuss the risks and benefits with the patient.

Parvovirus B19 infection may be serious for pregnant women (fetal infection) and for individuals with immunodeficiency or increased red blood cell turnover. Instruct patients to consult their physician if symptoms of B19 virus infection appear (fever, drowsiness, chills and runny nose followed about two weeks later by a rash and joint pain)[see *Pregnancy (8.1)*].

Manufactured For Baxter Healthcare Corporation

Deerfield, IL 60015 USA

US License No. 140

Baxter, Artiss Easyspray and Tisseel are registered trademarks of Baxter International Inc.

PACKAGE/LABEL PRINCIPAL DISPLAY PANEL

Fibrin Sealant (Human) NDC 0338-8503-01
ARTISS 2 mL Frozen
Baxter
Temperature sensitive – Do NOT expose above 37°C (99°F).

Contents:
Pre-filled syringe containing:
– **Sealer Protein Solution 1:** 1 mL, sterile
– Sealer Protein (Human)
– Fibrinolysis Inhibitor (Aprotinin, Synthetic), 3000 KIU/mL
– **Thrombin Solution 2:** 1 mL, sterile
– Thrombin (Human), 4 units/mL
– Calcium Chloride, 40 µmol/mL

**TOPICAL USE ONLY
DO NOT INJECT**
Read directions for thawing and application before use.
Store at –20°C (–4°F) or colder. Unopened pouches, thawed at room temperature, may be stored for up to 14 days at 15–25°C.
Do not refrigerate, microwave, or re-freeze.
Rx Only
Contents were sterilized and packaged under aseptic conditions.

Manufactured for Baxter
Healthcare Corporation
Deerfield IL, 60015 USA
U.S. License No. 140
0736601

DMC

Lot No.:
Exp. Date:
P

2 mL Pouch Label

Fibrin Sealant (Human) ARTISS 2 mL

NDC 0338-8503-01

Frozen

Baxter Logo

Temperature sensitive – Do NOT expose above 37°C (99°F).

Contents:

Pre-filled syringe containing:

- **Sealer Protein Solution 1:** 1 mL, sterile
- Sealer Protein (Human)
- Fibrinolysis Inhibitor (Aprotinin, Synthetic), 3000 KIU/mL

– **Thrombin Solution** □: **1 mL, sterile**

– Thrombin (Human), 4 units/mL

– Calcium Chloride, 40 µmol/mL

TOPICAL USE ONLY

DO NOT INJECT

Read directions for thawing and application before use.

Store at –20°C (–4°F) or colder. Unopened pouches, thawed at room temperature, may be stored for up to 14 days at 15 – 25°C.

Do not refrigerate, microwave, or re-freeze.

Rx Only

Contents were sterilized and packaged under aseptic conditions.

**Manufactured for Baxter
Healthcare Corporation**

Deerfield IL, 60015 USA

U.S. License No. 140

0736601

DMC

0736601

0100303388503010

Lot No.:

Exp. Date:

P

0103033885030272

07361602

Fibrin Sealant (Human)
ARTISS

TOPICAL USE ONLY

2 mL
Pre-filled Syringe



Baxter

Do not use on individuals with a known hypersensitivity to aprotin and/or any of the active substances or excipients.
The risks and benefits of this product should be discussed with the patient.
Read full prescribing information before use.
Store at -20°C (-4°F) or colder.
Unopened pouches, thawed at room temperature, may be stored for up to 14 days at 15-25°C.
Do not refrigerate, microwave, or re-freeze.
For single use only.
No preservative.
Not made with natural rubber latex.
Rx only.

TOPICAL USE ONLY
DO NOT INJECT

Vapor Heated, Solvent/Detergent Treated, Frozen

Fibrin Sealant (Human)
ARTISS

2 mL
Pre-filled Syringe

NDC 0338-8503-02



Contents:
Pre-filled syringe containing:
• Sealer Protein Solution: 1 mL, sterile
• Vapor Heated, Solvent/Detergent Treated
• Fibrinolytic Inhibitor (Aprotin, Synthetic), 3000 KIU/mL


• Thrombin Solution: 1 mL, sterile
• Thrombin (Human), 4 units/mL
• Vapor Heated, Solvent/Detergent Treated
• Calcium Chloride, 40 μmol/mL

Fibrin Sealant (Human)
ARTISS



2 mL
Pre-filled Syringe

TOPICAL USE ONLY

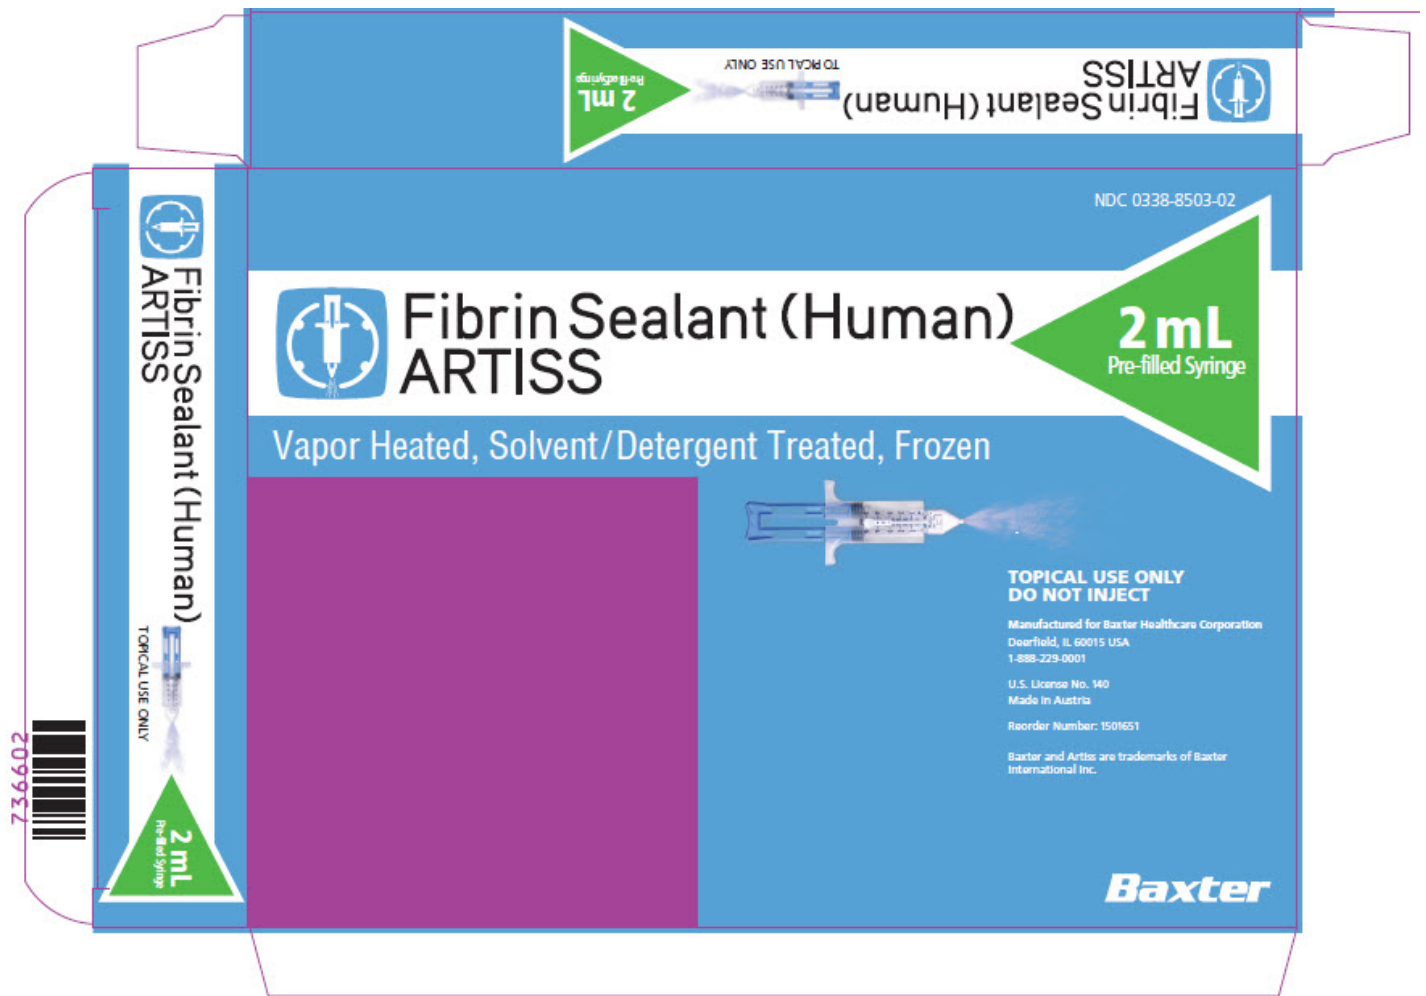

2 mL Carton Label

0736602

**Fibrin Sealant (Human)
ARTISS**

TOPICAL USE ONLY

2 mL
Pre-filled Syringe

N3 0338-8503-02 7

NDC 0338-8503-02 7

**Fibrin Sealant (Human)
ARTISS**

TOPICAL USE ONLY

2 mL
Pre-filled Syringe

Contents:

Pre-filled syringe containing:
Sealer Protein Solution: 1 mL, sterile

- Sealer Protein (Human)

Vapor Heated, Solvent/Detergent Treated

- Fibrinolysis Inhibitor (Aprotinin, Synthetic), 30000 KIU/mL

Thrombin Solution: 1mL, sterile

- Thrombin (Human), 4 units/mL
Vapor Heated, Solvent/Detergent Treated
- Calcium Chloride, 40 µmol/mL

**TOPICAL USE ONLY
DO NOT INJECT**

Do not use on individuals with a known hypersensitivity to aprotinin and/or any of the active substances or excipients.

The risks and benefits of this product should be discussed with the patient.

Read full prescribing information before use.

Store at -20°C (-4°F) or colder.

Unopened pouches, thawed at room temperature, may be stored for up to 14 days at 15 – 25°C.

Do not refrigerate, microwave, or re-freeze.

For single use only

No preservative

Not made with natural rubber latex

Rx only

Baxter Logo

**Fibrin Sealant (Human)
ARTISS**

TOPICAL USE ONLY

2 mL
Pre-filled Syringe

**Fibrin Sealant (Human)
ARTISS**

TOPICAL USE ONLY

736602

**Fibrin Sealant (Human)
ARTISS**

TOPICAL USE ONLY

2 mL
Pre-filled Syringe

2 mL
Pre-filled Syringe

NDC 0338-8503-02

Fibrin Sealant (Human)

ARTISS

TOPICAL USE ONLY

2 mL

Pre-filled Syringe

Vapor Heated, Solvent/Detergent Treated, Frozen

TOPICAL USE ONLY

DO NOT INJECT

Manufactured for Baxter Healthcare Corporation

Deerfield, IL 60015 USA

1-888-229-0001

U.S. License No. 140

Made in Austria

Reorder Number: 1501651

Baxter and Artiss are trademarks of Baxter International Inc.

Baxter Logo



DUO Set A 2 ml / 4 ml Label

Baxter Logo

DUO Set A 2 ml / 4 ml

Indications for Use:

For the application of ARTISS Fibrin Sealant

For single use only. Not made with natural rubber latex.

Do not reuse or resterilize. Sterilized by gamma radiation.

Sterile and non-pyrogenic in unopened and undamaged package.

Rx Only.

Manufactured for:

Baxter Healthcare Corporation

One Baxter Parkway

Deerfield, IL 60015 USA

Made in Belgium

Lot No.

Exp. Date:

REF

BE-90-01-042

ARTISS FIBRIN SEALANT

fibrinogen human, human thrombin solution

Product Information

Product Type	PLASMA DERIVATIVE	Item Code (Source)	NDC:0338-8503
Route of Administration	TOPICAL		

Active Ingredient/Active Moiety

Ingredient Name	Basis of Strength	Strength
FIBRINO GEN HUMAN (UNII: N94833051K) (FIBRINOGEN HUMAN - UNII:N94833051K)	FIBRINOGEN HUMAN	90 mg in 1 mL
HUMAN THROMBIN (UNII: 6K15ABL77G) (HUMAN THROMBIN - UNII:6K15ABL77G)	HUMAN THROMBIN	4 [iU] in 1 mL

Inactive Ingredients

Ingredient Name	Strength
APROTININ (UNII: 04XPW8C0FL)	
CALCIUM CHLORIDE (UNII: M4I0D6VV5M)	
ALBUMIN HUMAN (UNII: ZIF514RVZR)	
TRISODIUM CITRATE DIHYDRATE (UNII: B22547B95K)	
HISTIDINE (UNII: 4QD397987E)	
NIACINAMIDE (UNII: 25X51I8RD4)	
POLYSORBATE 80 (UNII: 6OZP39ZG8H)	
SODIUM CHLORIDE (UNII: 451W47IQ8X)	
WATER (UNII: 059QF0KO0R)	

Packaging

#	Item Code	Package Description	Marketing Start Date	Marketing End Date
---	-----------	---------------------	----------------------	--------------------

1	NDC:0338-8503-02	1 in 1 CARTON		
1	NDC:0338-8503-01	2 mL in 1 SYRINGE, PLASTIC; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		
2	NDC:0338-8503-04	1 in 1 CARTON		
2	NDC:0338-8503-03	4 mL in 1 SYRINGE, PLASTIC; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		
3	NDC:0338-8503-10	1 in 1 CARTON		
3	NDC:0338-8503-09	10 mL in 1 SYRINGE, PLASTIC; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		

Marketing Information

Marketing Category	Application Number or Monograph Citation	Marketing Start Date	Marketing End Date
BLA	BLA125266	03/19/2008	

Labeler - Baxter Healthcare Corporation (005083209)

Establishment

Name	Address	ID/FEI	Business Operations
Baxter Aktiengesellschaft		300434671	MANUFACTURE(0338-8503)

Establishment

Name	Address	ID/FEI	Business Operations
Baxter Aktiengesellschaft		300466733	ANALYSIS(0338-8503)

Revised: 12/2019

Baxter Healthcare Corporation