

**Rebif® Rebidose®**

**Instructions For Use**



**Exclusively for use with**

**Rebif®**  
(interferon beta-1a)  
subcutaneous injection

## Welcome

This guide contains information on how to use Rebif® Rebidose®, a pre-assembled, single-use autoinjector that administers one dose of Rebif® (interferon beta-1a) for the treatment of relapsing forms of multiple sclerosis.


See the Full Prescribing Information for information about Rebif, including risks associated with the drug such as suicide and depression, hepatic injury, and injection site reactions.

Please read these instructions carefully before you start using the Rebif® Rebidose® and remember, you must have received the appropriate training before injecting.

If at any time, you have questions or concerns, please contact your health care provider or call MS LifeLines at 1-877-447-3243.

## Rx Only

## Contents


Rebif® Rebidose® features.....	4
 Warnings.....	6
Important Information.....	8
How Supplied.....	10
Titration.....	12
Recording your injections.....	13
Choosing an injection site.....	18
Step 1: Prepare for your injection.....	20
Examine syringe and expiration date.....	21
Step 2: Administer your injection.....	24
Step 3: Finish your injection.....	26
Disposal.....	28
Storage.....	31
Travel.....	32

### Rebif® Rebidose® features

Before injection:



After injection:

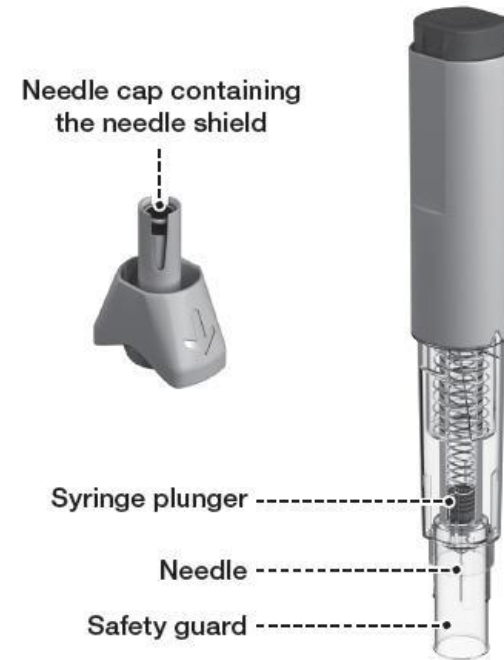

### Warnings

- Always use the injection technique advised by your health care provider and contact them with any questions you might have.
- Always keep the Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector out of the reach of children.
- **Do not** share your autoinjector with anyone. Doing so may result in injury, including the transmission of infectious blood-borne diseases. Adhere to strict safety and antiseptic precautions at all times.
  - **Do not** insert your fingers into the opening of the safety guard.
  - **Do not** try to re-use a Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector that has already been used.
  - Adhere to proper disposal procedures to avoid a needle stick injury.

### Warnings

- Check the expiration date on the Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector label and its carton. If the medication has expired, **Do not** use it.
- Examine the contents of the syringe carefully through the transparent housing. The liquid should be clear or slightly yellow. Inspect for cracks or breakage in the syringe or other parts. **Do not** use Rebidose<sup>®</sup> if it is cracked or broken or if the liquid is cloudy, discolored or contains particles.
- If the Rebidose<sup>®</sup> has been dropped more than 3 feet, or if it looks damaged for any reason, **Do not** use it. Instead, dispose of it in an acceptable biohazard (sharps) container and use a new Rebidose<sup>®</sup> autoinjector.
- Contact your health care provider about any damaged Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector.

## Important Information

- Store your Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjectors in a refrigerator until ready for use.
- If you or someone around you is injured by the needle, contact your health care provider immediately and dispose of the Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector in an acceptable biohazard (sharps) container.
- Injecting Rebif<sup>®</sup> the medicine using the Rebidose<sup>®</sup> autoinjector may cause skin reactions including soreness, redness, pain, bruising, or swelling. Tell your health care provider about any skin reactions that become swollen, painful, or look infected and do not heal within a few days.
- Use a different site each time you inject. **Do not** inject Rebif<sup>®</sup> where your skin is irritated, reddened, bruised, infected or abnormal in any way.
- The Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector contains a glass syringe. In very rare cases, the syringe may break during the injection. If this happens, immediately dispose of any broken glass and the damaged Rebidose<sup>®</sup> autoinjector in the biohazard (sharps) container, taking necessary precautions to avoid injury. Contact your health care provider or MS LifeLines at 1-877-447-3243 immediately.

## How Supplied

Rebif® Rebidose® is available in 3 dose sizes. Check that the dose of Rebif® is the one prescribed for you by looking at the Rebidose® carton and at the dose label on the Rebidose® autoinjector.

Rebif® Rebidose® autoinjectors are supplied in these 3 packaging presentations:

- Titration Pack
  - 6 Rebif® 8.8 mcg Rebidose® autoinjectors with a lime green injector button.
  - 6 Rebif® 22 mcg Rebidose® autoinjectors with a yellow injector button.
- 12 Rebif® 22 mcg Rebidose® autoinjectors with a yellow injector button.
- 12 Rebif® 44 mcg Rebidose® autoinjectors with a teal green injector button.



## Titration

At the beginning of Rebif® treatment, your health care provider may prescribe a titration phase to gradually increase to the intended dosage.

The Rebif® Rebidose® Titration Pack contains six 8.8 mcg autoinjectors with a lime green injector button and six 22 mcg autoinjectors with a yellow injector button.

The titration period lasts 4 weeks and during this time, you will administer 12 injections:

- **Weeks 1 and 2:** Use one 8.8 mcg autoinjector three times a week, at least 48 hours apart.
- **Weeks 3 and 4:** Use one 22 mcg autoinjector three times a week, at least 48 hours apart.

Your health care provider may provide a different dose and schedule.

## Recording your injections

You may find it helpful to record information about your 3 weekly injections to discuss with your health care provider.

You can record your injections:

- By hand, using a tracking sheet (see page 14)
- By scan, using the MSdialog Mobile App that can see or scan information from your autoinjector's label (see page 15)

Contact your health care provider or MS LifeLines at 1-877-447-3243 for information about recording options.

*Recording your injections (continued)*


**Use tracking sheet**

Week 1	Inj. Site	Date & Time	Site Reaction	
Inj. 1			Yes	No
Inj. 2			Yes	No
Inj. 3			Yes	No
Week 2	Inj. Site	Date & Time	Site Reaction	
Inj. 1			Yes	No
Inj. 2			Yes	No
Inj. 3			Yes	No
Week 3	Inj. Site	Date & Time	Site Reaction	
Inj. 1			Yes	No
Inj. 2			Yes	No
Inj. 3			Yes	No
Week 4	Inj. Site	Date & Time	Site Reaction	
Inj. 1			Yes	No
Inj. 2			Yes	No
Inj. 3			Yes	No

**Use MSdialog Mobile App**

If you have an Apple iPhone® or Google Android™ smartphone, you can use the MSdialog Mobile App to record your injections.

The Rebif® Rebidose® autoinjector label features a **2D code** and a **Near-Field Communication (NFC) tag**. The MSdialog Mobile App can scan the code or tag to record information about the autoinjector.

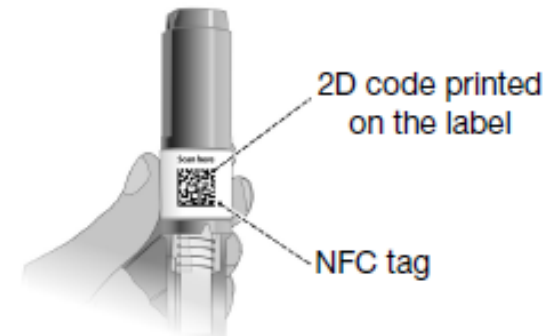

Apple and iPhone are trademarks of Apple Inc. and Google and Android are trademarks of Google Inc.

*Recording your injections (continued)*


**Choose one of the following two options:**

**Option 1: Scan 2D code**



- 1) Point the smartphone's camera at the autoinjector's label, centering the 2D code in the application's viewing window.
- 2) Hold the smartphone steady until it makes a sound or vibrates, indicating that the 2D code has been scanned.

**Option 2: Read NFC tag**

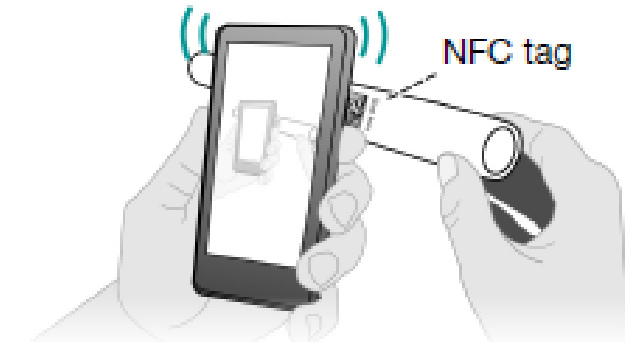

- 1) Hold the NFC tag against the back of the smartphone, making sure the label contacts the smartphone's back.
- 2) Hold the smartphone steady until it makes a sound or vibrates, indicating that the NFC tag has been read.

### Choosing an injection site


The best sites for giving a subcutaneous injection are those areas with a layer of fat between the skin and muscle. These include the thigh, the outer surface of the upper arm, the stomach and the buttocks.

**Do not** use the area near your waistline or within 2 inches of your navel.

Only choose one site for injection. Use a different site each time you inject.

#### **Caution**

**Do not** inject Rebif® where your skin is irritated, reddened, bruised, infected or abnormal in any way.

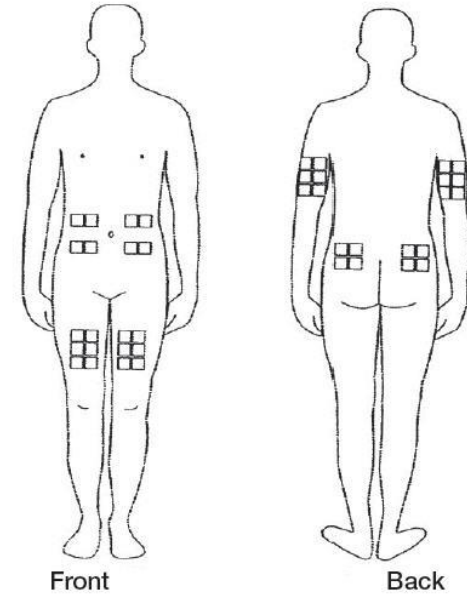

### Step 1: Prepare for your injection

1.1) Before you begin, you may find injecting more comfortable if you allow time for the Rebif<sup>®</sup> to warm up to room temperature before injecting. Therefore, it is recommended that you remove the Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector from the refrigerator at least 30 minutes prior to use.

#### **Caution**

**Do not** heat or microwave a Rebidose<sup>®</sup> autoinjector.

1.2) Put all of the items listed below within easy reach on a table or other stable surface:

- 1 Rebidose<sup>®</sup> autoinjector containing Rebif<sup>®</sup>
- Alcohol wipes/swabs or cotton balls and rubbing alcohol
- Small adhesive bandage strip (if needed)
- A biohazard (sharps) container (see Disposal section on page 28)

1.3) Wash your hands thoroughly with antibacterial soap.

1.4) Open the tray over a table or soft surface by peeling back the plastic covering and remove 1 Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector. **Do not** remove the needle cap until you are ready to inject because the autoinjector could roll off the table and become unsterile.

1.5) Check the expiration date on the Rebidose<sup>®</sup> autoinjector label and its carton. If the medication has expired, **do not** use it.

1.6) Examine the contents of the syringe carefully through the transparent housing. The liquid should be clear or slightly yellow.

1.7) Inspect for cracks or breakage in the syringe or other parts. **Do not** use the Rebif<sup>®</sup> Rebidose<sup>®</sup> autoinjector if it is cracked or broken or if the liquid is cloudy, discolored or contains particles.

*Step 1: Prepare for your injection (continued)*

1.8) Use an alcohol wipe to clean the injection site. Let your skin dry to prevent stinging during injection.


1.9) Hold the Rebidose<sup>®</sup> by the injector body (fig **a**) and pull off the needle cap.

1.10) Look inside the needle cap to make sure you see a black needle shield inside the cap (fig **b**).

1.11) Dispose of the needle cap and proceed to the injection step without delay.

**⚠ Warning**

If the Rebidose<sup>®</sup> has been dropped more than 3 feet, or if it looks damaged for any reason, **do not** use it. Instead, dispose of it in an acceptable biohazard (sharps) container and use a new Rebidose<sup>®</sup> autoinjector.

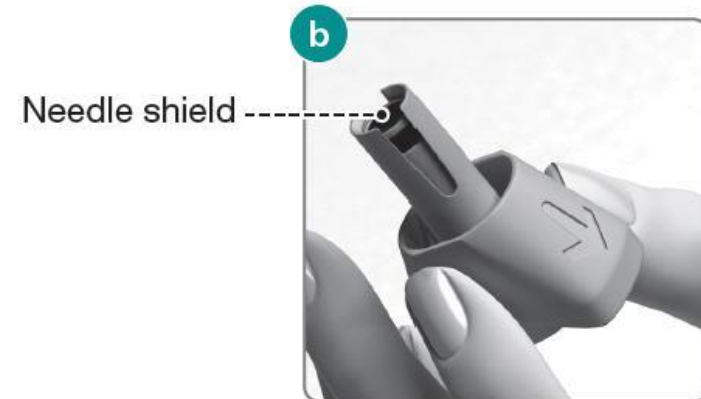


## Step 2: Administer your injection

2.1) Hold the Rebidose<sup>®</sup> autoinjector in your palm with your thumb above the injector button.

2.2) Place the Rebidose<sup>®</sup> upright with the needle end flat against your skin at a 90° angle. Push the Rebidose<sup>®</sup> against your skin until you feel resistance; this action unlocks the injector button (fig **c**).

2.3) Keep the Rebidose<sup>®</sup> pressed firmly against the skin and use your thumb to push the injector button (fig **d**). You will hear a click, which means the injection has begun.

2.4) Keep the Rebidose<sup>®</sup> pressed firmly against your skin for at least 10 seconds while the medication is dispensed (fig **e**).

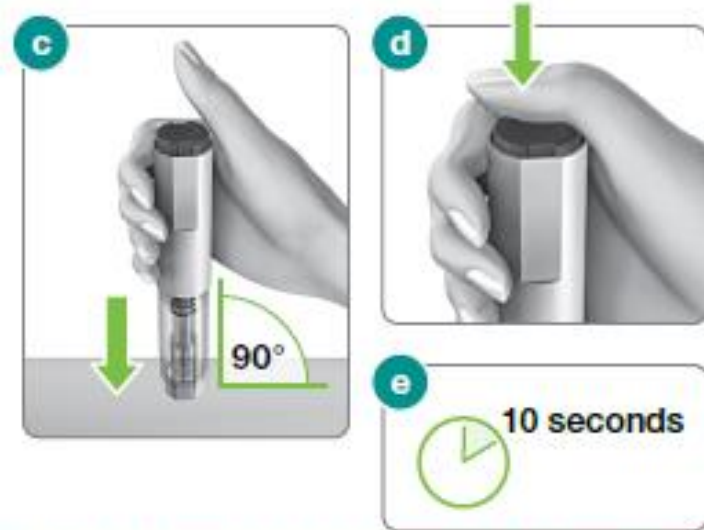

### ⚠ Caution

If the injection does not start, release the injector button and make sure that the Rebidose<sup>®</sup> is still pressed firmly against your skin. Then push firmly on the injector button, listening for the click that indicates the start of the injection.


### Step 3: Finish your injection

3.1) Before lifting the Rebidose<sup>®</sup> from your skin, make sure that the syringe plunger has moved to the bottom and that the entire dose has been injected (fig f).

3.2) Lift the Rebidose<sup>®</sup> from the injection site. The safety guard slides down and locks into place to protect you from the needle (fig g). If any liquid is left in the syringe or if you have any other problems, contact your health care provider or MS LifeLines at 1-877-447-3243.

**Do not** try to put the needle cap on the used Rebidose<sup>®</sup> autoinjector. It is no longer needed.

3.3) If desired, use a small adhesive bandage to cover the injection site.

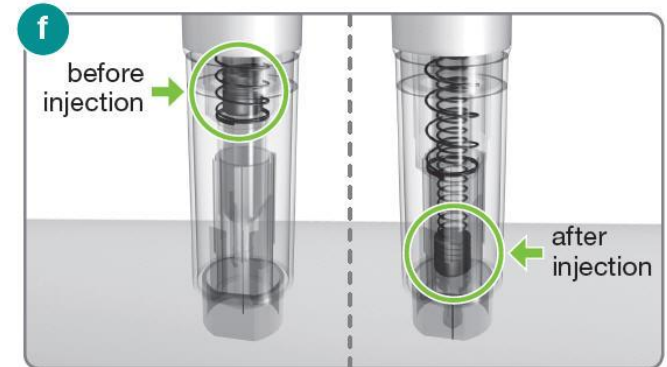

## Disposal

1) Put your used Rebidose<sup>®</sup> autoinjectors in a FDA-cleared sharps disposal container right away after use (fig h). Do not throw them away (dispose of) in your household trash.



2) If you do not have a FDA-cleared sharps disposal container, you may use a household container that is:

- made of a heavy-duty plastic;

- can be closed with a tight-fitting, puncture-resistant lid, without sharps being able to come out;
- upright and stable during use;
- leak-resistant; and
- properly labeled to warn of hazardous waste inside the container.

3) When your sharps disposal container is almost full, you will need to follow your community guidelines for the correct way to dispose of it. There may be state or local laws about how you should throw away used needles and syringes. For more information about safe sharps disposal in the state that you live in, go to the FDA's website at: <http://www.fda.gov/safesharpsdisposal>

4) Do not dispose of your used sharps disposal container in your household trash unless your community guidelines permit this. Do not recycle your used sharps disposal container.

*Disposal (continued)*

 **Caution**

Always keep the biohazard (sharps) container out of the sight and reach of children.

 **Warning**

- **Do not** insert your fingers into the opening of the safety guard.
- **Do not** try to re-use a Rebidose<sup>®</sup> single-use autoinjector that has already been used.
- Adhere to proper disposal procedures to avoid a needle stick injury.

**Storage**

- Each Rebidose<sup>®</sup> autoinjector contains a single dose of Rebif<sup>®</sup>.
- Store Rebidose<sup>®</sup> autoinjectors in the refrigerator between 36°F and 46°F (2°C to 8°C). **Do not freeze**. If a refrigerator is not available, Rebidose<sup>®</sup> may be stored between 36°F and 77°F (2°C to 25°C) for up to 30 days away from heat and light.
- **Do not** put them in or near the freezer compartment. **Do not** inject Rebif<sup>®</sup> that you know or suspect has been frozen.
- Keep the Rebidose<sup>®</sup> in its packaging and only open one when you need it. Refer to the Rebif<sup>®</sup> drug package insert and medication guide for specific storage guidelines.

## Travel

- When you travel, take 3 Rebidose<sup>®</sup> autoinjectors with you for each week of your trip. Take some extra in case you are away for longer than expected.
- Remember to pack an empty biohazard (sharps) container for proper disposal.
- When traveling by air, always carry Rebidose<sup>®</sup> autoinjectors in your hand luggage because the aircraft luggage compartment can be very cold and the Rebidose<sup>®</sup> could freeze.
- It is safe to pass Rebidose<sup>®</sup> autoinjectors through x-ray machines, but you may need a note from your health care provider to allow you to carry them aboard an airplane.
- Prior to traveling, always check with your airline and your health care provider about bringing injectable medication with you.

This page intentionally  
left blank.

This label may not be the latest approved by FDA.  
For current labeling information, please visit <https://www.fda.gov/drugsatfda>

This Instructions for Use has been approved by  
the Food and Drug Administration.

Version: September 27, 2016  
Manufactured for: EMD Serono, Inc.  
Rockland, MA 02730 U.S. Lic. 1773  
MS LifeLines: 1-877-447-3243